

The development of a “reduced logMAR” visual acuity chart for use in routine clinical practice

D A Rosser, D A H Laidlaw, I E Murdoch

Abstract

Background/claims—The advantages of logMAR acuity data over the Snellen fraction are well known, and yet existing logMAR charts have not been adopted into routine ophthalmic clinical use. As this may be due in part to the time required for a logMAR measurement, this study was performed to determine whether an abbreviated logMAR chart design could combine the advantages of existing charts with a clinically acceptable measurement time.

Methods—The test-retest variability, agreement (with the gold standard), and time taken for “single letter” (interpolated) acuity measurements taken using three prototype “reduced logMAR” (RLM) charts and the Snellen chart were compared with those of the ETDRS chart which acted as the gold standard. The Snellen chart was also scored with the more familiar “line assignment” method. The subjects undergoing these measurements were drawn from a typical clinical outpatient population exhibiting a range of acuities.

Results—The RLM A prototype chart achieved a test-retest variability of ± 0.24 logMAR compared with ± 0.18 for the ETDRS chart. Test-retest variability for the Snellen chart was ± 0.24 logMAR using clinically prohibitive “single letter” scoring increasing to ± 0.33 with the more usual “line assignment” method. All charts produced acuity data which agreed well with those of the ETDRS chart. “Single letter” acuity measurements using the prototype RLM charts were completed in approximately half the time of those taken using the ETDRS and Snellen charts. The duration of a Snellen “line assignment” measurement was not evaluated.

Conclusion—The RLM A chart offers an acceptable level of test-retest variability when compared with the gold standard ETDRS chart, while reducing the measurement time by half. Also, by allowing a faster, less variable acuity measurement than the Snellen chart, the RLM A chart can bring the benefits of logMAR acuity to routine clinical practice.

(*Br J Ophthalmol* 2001;85:432-436)

clinical use, the measurement error (test-retest variability or TRV) of acuity should be both consistent across the acuity range and quantifiable in terms of lines or letters of change. The Snellen chart,¹ although being the commonest tool for the measurement of visual acuity in ophthalmic practice, exhibits certain well documented design flaws²⁻⁶ which may compromise its usefulness in this respect. Firstly, the non-geometric progression of letter sizes and the variable number of letters per line prevents TRV from being specified in terms of letters or lines of change.

Also, the lack of a systematic approach to letter legibility and crowding may compromise the reliability of Snellen measurements as letter size is not the sole determinant of the difficulty of a given line of letters. Furthermore, in being ordinal data rather than interval data, the Snellen fraction notation is not easily subjected to statistical analysis, and does not lend itself to an interpolated method of acuity scoring which is known to provide lower TRV than the “line assignment” method more usually employed with the Snellen chart^{7,8} (see “Scoring” in the “Materials and methods” section for definitions of scoring methods).

These theoretical design problems were addressed with the development of logMAR acuity charts^{2,9,10} which are now frequently employed in prospective clinical research. LogMAR charts, however, have not been widely adopted into routine clinical practice. This may be due to the unfamiliar scoring system, the chart’s size, and the perception of a logMAR measurement as being time consuming.

We hypothesise that a logMAR chart with a reduced number of letters per line would allow measurements to be made in a clinically acceptable period of time, and with greater precision and reliability than is possible with Snellen charts. The performance of three different prototype charts (“reduced logMAR” or “RLM” charts A, B, and C) was compared, in terms of TRV and measurement time, with that of the Snellen chart, as well as the ETDRS (Early Treatment Diabetic Retinopathy Study) logMAR chart,¹⁰ which acted as the gold standard.

Materials and methods

SUBJECTS

Patients who fulfilled the following inclusion criteria were recruited from the primary care and cataract clinics of Moorfields Eye Hospital:

- Snellen acuity of between 6/5 and 6/60
- a diagnosis of cataract, pseudophakia, or early glaucoma (no visual field defects in the central 20°)

Optometry
Department,
Moorfields NHS Trust,
City Road, London
EC1V 2PD, UK
D A Rosser

Vitreoretinal Unit, St
Thomas’s Hospital,
Lambeth Palace Road,
London SE1 7EH
D A H Laidlaw

Department of
Epidemiology and
International Eye
Health, Institute of
Ophthalmology,
University College
London, Bath Street,
London EC1V 9EL
D A Rosser
I E Murdoch

Correspondence to:
D A Rosser
dan@drosser.freereserve.co.uk

Accepted for publication
4 October 2000

The most common clinical measurement of visual function is visual acuity. It is used to determine the need for, and outcome of, many interventions as well as to monitor the course of eye disease. It is therefore desirable that for

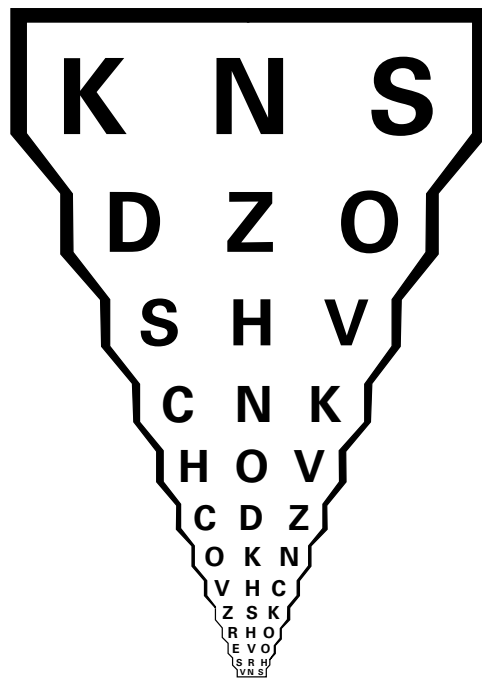


Figure 1 The RLM A chart.

(c) able to understand and comply with the testing protocol.

One eye of each subject was assessed. Where both eyes met the criteria, the eye with the poorest acuity was used as the study eye.

A total of 16 male and 25 female subjects aged 49–89 years were recruited: 30 subjects had cataract, seven were pseudophakic, and four had primary open angle glaucoma. Acuities ranged from +0.82 to -0.14 (median +0.34) logMAR.

THE CHARTS

Two versions of each of the five different chart designs were used in the study. The chart design parameters and the acuity range at a 6 metre testing distance are summarised in Table 1.

Reduced logMAR (RLM) charts

These prototype charts conformed to the design principles used in the ETDRS chart¹⁰ in terms of logarithmic letter size progression, interletter spacing, interline spacing, the avoidance of words or acronyms, and the use of the Sloan set of letters.⁹ In view of the fact that letter recognition measurements in both normals and abnormals can be influenced by the proximity of the letter to any surrounding contours,¹¹ all the RLM charts were surrounded by a continuous "crowding bar" (see Fig 1). This

Table 1 Summary of chart design

Chart	No of letters per line	Line interval in logMAR	Single letter value in logMAR	Total No of letters	Acuity range at 6 metres
ETDRS	5	0.1	0.02	120	+0.82 to -0.48
RLM A	3	0.1	0.033	39	+0.72 to -0.48
RLM B	2	0.1	0.05	26	+0.72 to -0.48
RLM C	3	0.15	0.05	27	+0.72 to -0.48
Snellen	1 to 8	0.08 to 0.22	0.01 to 0.11	45	+1.0 to -0.18

The number of letters per line, line interval and single letter value are constant throughout for each chart design except the Snellen chart where the range of values has been given.

was employed to compensate for the reduction in the proportion of letters crowded from both sides produced by reducing the number of letters per line. The bar was positioned 2.5 stroke widths (half a letter) from the edge of the letters as the difficulty of letters crowded in this way has been shown to equate well to that of letters in a linear arrangement.¹²

ETDRS charts (Lighthouse Low Vision Products)

ETDRS charts 1 and 2 were used. The refraction chart was used for patient demonstration purposes.

The Snellen Charts (Clement Clarke UK)

The two Snellen charts used were selected to be as similar as possible and, in order to reduce truncation effects, included a 6/4 line.

CHART DISPLAY

The RLM charts and the ETDRS charts were displayed in the standard Lighthouse light box. The Snellen charts were displayed in the standard Clement Clark light box. All charts were backlit in the appropriate light boxes.

TESTING PROTOCOL

Timed acuity measurements were taken on one eye of each subject, one measurement being taken using both versions of each of the five chart types. The time was measured from the subject starting to read the letters until they had made a complete line of errors. Calculation of acuity scores was performed separately to avoid influencing the time measurements. The charts were viewed in random order and responses were recorded on specially designed data proformas.

All measurements were conducted by a single examiner using a forced choice paradigm under consistent lighting conditions. All subjects wore their habitual spectacle correction. All charts were read from a distance of 6 metres unless the subject misnamed any letters on the top line of a given chart. In this event, the subject was moved to 1.5 metres and the remainder of the measurements were taken at this distance. The end point for each chart was defined as an entire line of letters being misread or, in the case of some letters being read on the bottom line, all the letters on the chart having been attempted.

SCORING

The Snellen acuity data (from 6/4 to 6/60) were converted to the logMAR format. This is done by taking the log to the base 10 of the reciprocal of the Snellen acuity fraction. This transform can be performed regardless of the denominator or numerator.

eg, 6/9 → 9/6 = 1.5 then $\log(1.5) = +0.18$ logMAR

An interpolated logMAR acuity score ("single letter" score) was produced for each chart using the formula

$$1.10 - T_c L_v$$

where T_c is the total number of correctly named letters and L_v is the logMAR value of each letter on the chart. The individual letter

Table 2 Test-retest variability of the five chart designs

Chart	Mean difference	95% confidence interval for the mean	SD	95% CI for agreement
ETDRS 1 – ETDRS 2	0.00	-0.03 to +0.03	0.09	-0.18 to +0.18
RLM A 1 – RLM A 2	+0.01	-0.03 to +0.05	0.12	-0.24 to +0.24
RLM B 1 – RLM B 2	-0.03	-0.08 to +0.02	0.16	-0.31 to +0.31
RLM C 1 – RLM C 2	-0.01	-0.05 to +0.03	0.14	-0.27 to +0.27
Snellen 1 – Snellen 2 (single letter)	+0.01	-0.03 to +0.05	0.12	-0.24 to +0.24
Snellen 1 – Snellen 2 (Line assignment)	-0.02	-0.07 to +0.03	0.17	-0.33 to +0.33

The figures show the level of test-retest variability of each chart design as determined using the methods of Bland and Altman. The Snellen "line assignment" scores were used to calculate the bottom row of figures, otherwise "single letter" scoring is used throughout.

values are produced by dividing the logMAR interval between a given line and the line below by the number of letters on that line.¹⁰ Each letter on the ETDRS and reduced logMAR charts therefore has an equal value, whereas the value of a Snellen letter will depend on which line it is presented.

The Snellen charts were also scored using a "line assignment" method, this being the most common method by which Snellen acuity data are produced in clinical practice. The acuity score was defined as the value of the lowest line on which at least half of the letters were named correctly.

All acuity scores were adjusted for testing distance before analysis.

METHOD OF ANALYSIS

Our objectives were as follows:

- to determine in terms of mean difference and 95% confidence intervals, the TRV of single letter acuity data using each of the five chart designs, as well as the TRV of a Snellen line assignment measurement
- to determine in terms of mean difference and 95% confidence intervals, the extent to which measurements taken using the reduced logMAR and Snellen charts agreed with the gold standard ETDRS chart and
- to compare the time taken to perform a "single letter" measurement on each chart. The methods of Bland and Altman¹³ were used to determine (a) and (b) above.

Results

Histograms of the distribution of the test-retest and interchart acuity variability data suggested that these data conformed to a normal distribution. Scatter plots of difference in acuity verses mean acuity¹³ suggested that there were no systematic associations within any of these data sets between the extent of the agreement or TRV and the underlying acuities.

Table 2 shows the ETDRS chart to produce acuities with the lowest (best) TRV with 95% confidence limits for agreement of ± 0.18 logMAR. The RLM A and Snellen "single letter" measurements were more variable, both

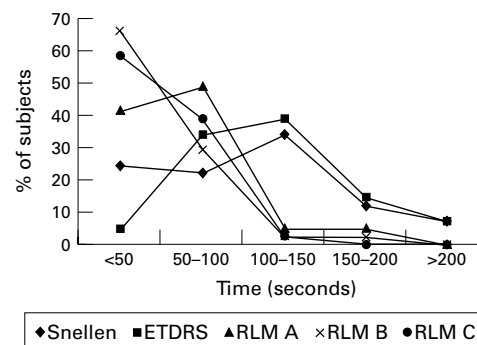


Figure 2 "Single letter" chart reading times.

with figures of ± 0.24 logMAR; and the TRV for the RLM C, RLM B, and Snellen "line assignment" acuities were higher still (± 0.27 , ± 0.31 , and ± 0.33 respectively).

Table 3 shows that the acuities recorded using the RLM charts did not exhibit any systematic bias when compared with the ETDRS chart. Good agreement is indicated by the 95% confidence intervals for the mean including zero. Snellen acuities showed no systematic bias providing they were scored with the "single letter" scoring method.

Figure 2 is a graphical representation of the chart reading times. It can be seen that a high proportion of chart readings using the RLM A, B, and C charts were completed in less than 50 seconds (41%, 66%, and 59% respectively), while very few require more than 100 seconds (10%, 4%, and 2%). Conversely for the ETDRS and Snellen charts, fewer chart readings are completed in under 50 seconds (5% and 24% respectively), a high proportion require between 100 and 150 seconds (39% and 34%), and some more than 200 seconds (7% and 7%). Table 4 shows the chart reading times for the RLM charts to be approximately half to a third of those for the ETDRS and Snellen charts across the distribution; the only exception being where the very shortest times were similar for both the RLM and Snellen charts.

Table 3 Agreement with ETDRS measurements

Chart	Mean difference	95% CI for the mean	SD	95% CI for agreement
ETDRS 1 – RLM A 1	0.00	-0.03 to +0.03	0.10	-0.20 to +0.20
ETDRS 1 – RLM B 1	+0.01	-0.03 to +0.05	0.12	-0.24 to +0.24
ETDRS 1 – RLM C 1	-0.01	-0.05 to +0.03	0.12	-0.24 to +0.24
ETDRS 1 – Snellen 1 (single letter)	+0.02	-0.02 to +0.06	0.14	-0.27 to +0.27

The figures show the level of agreement between each pair of chart designs in the first column as determined using the methods of Bland and Altman. "Single letter" scoring is used throughout.

Table 4 Reading time for each of the five chart designs

Chart	Minimum	25th centile	Median	75th centile	Maximum
ETDRS	41	79	106	147	405
RLM A	13	42	59	75	182
RLM B	14	22	34	54	161
RLM C	19	34	47	70	104
Snellen	19	70	110	161	417

Figures are time taken in seconds to complete a chart reading—that is, measurement time excluding score calculation time.

Discussion

Our aim was to develop a logMAR chart which:

- produced a consistent and acceptable level of TRV across a range of acuities
- produced acuity data which agreed well with those of the ETDRS chart
- could be used in a clinically acceptable period of time and
- produced interval acuity data.

The Bland and Altman scatter plots of difference versus mean referred to in the results section demonstrated that for all the charts, agreement and TRV were consistent across the range of acuities featured in this study.

The ETDRS TRV found in this study (± 0.18 logMAR) is in keeping with previously reported data using the ETDRS or Bailey-Lovie charts which range from ± 0.09 to ± 0.20 logMAR.^{6,7,14-17} Cataract, uncorrected refractive error, and the use of non-practised observers are known to have a detrimental effect on TRV^{6,15} and may account for the higher variability in our study (which used habitual spectacle correction) compared with some of those shown above. The results allow us to compare the performance of the different charts within the same population. Table 2 shows the test-retest variability of the RLM A chart (± 0.24 log units) to compare favourably with that of the ETDRS chart (± 0.18 log units); while the TRV of the RLM B and C charts was larger still (± 0.31 and ± 0.27 log units respectively). The increased variability obtained with the prototype charts can be accounted for by the larger scale interval (single letter value) compared with that of the ETDRS chart⁷ (see Table 1). Scoring the Snellen chart with the “line assignment” method produces the largest scale intervals and hence the highest TRV (± 0.33 log units). The Snellen single letter method produced the same TRV as the RLM A chart, but is too time consuming for clinical use, as will be discussed later.

Table 3 shows that the acuities recorded using the RLM charts showed good agreement with those recorded using the ETDRS chart suggesting that none of our modifications to the ETDRS format had introduced any systematic bias to the data. Snellen acuities also showed good agreement with ETDRS acuities when scored with the “single letter” scoring method.

In interpreting the chart reading time data, it should be remembered that all times refer to “single letter” acuity measurements. The line assignment method commonly used with the Snellen chart in clinical practice may allow

quicker measurements. This would be expected because, unlike the single letter method, the line assignment method does not require that the patient continues to attempt letters until they have misnamed all of the letters on one line (a forced choice testing paradigm). Instead, the test is terminated either when half or more of the letters are misread or, more typically, when the patient states that (in their opinion) they cannot read any letters on the next line, which is then not attempted. Hence, not only is the single letter measurement likely to require more letters to be attempted but, also, the additional letters are of a size close to the patients threshold which are typically more time consuming to attempt. The study design did not allow for the duration of a Snellen “line assignment” measurement to be assessed because to note measurement time at two separate end points was deemed excessively complicated.

The data displayed in Figure 2 clearly show a tendency for “single letter” measurements taken using the RLM charts to be less time consuming than those taken using the ETDRS and Snellen charts. The likely explanation for this is, firstly, the reduced total number of letters, but also that fewer letters per line will reduce the number of letters at or around threshold which are typically more time consuming to attempt. A slowing of responses at threshold may account for the shorter measurement times for RLM B compared with RLM C, these two charts having an almost identical total number of letters (see Table 1) but the former having only two letters per line. RLM A measurements are slightly more time consuming than RLM B and RLM C, as the total number of letters and/or number of letters per line is higher.

The median “single letter” chart reading times for the RLM A chart were approximately half of the corresponding times for both the ETDRS chart and the Snellen chart (see Table 4). The only exceptions to this were the shortest Snellen chart reading times, which were almost as short as those for the RLM A chart. A plot of chart reading time against acuity for the Snellen chart showed the shortest measurement times to be those related to the poorest acuities where only a small number of letters at the top of the Snellen chart had been attempted.

The time data in Figure 2 and Table 4 represent the duration of “single letter”, forced choice measurement times exclusive of score calculation—that is, *chart reading time* only. Score calculation was carried out separately so as to prevent this acting as a confounding variable. It should be noted that the calculation of a Snellen “single letter” score requires approximately 1 minute in addition to the time required for the subject to read the chart. It also requires reference to be made to a set of tables and/or the use of a calculator. This would clearly be impractical in a clinical setting. For the ETDRS and RLM charts, calculation of a single letter score takes approximately 10 seconds.

Conclusion

Snellen line assignment measurements are very variable, whereas Snellen single letter measurements are slow and clinically impractical. Although measurements taken using contemporary logMAR charts such as the ETDRS are subject to a low level of TRV, they are time consuming. This may explain why, more than 20 years after their development, these superior charts have still not been widely adopted into routine clinical practice. An abbreviated design of logMAR chart can offer the format of the pre-existing logMAR charts with the inherent benefits concerning scoring and analyses as well as consistent TRV with which to identify clinically significant change. Measurements taken using the RLM A chart design were found to be slightly more variable (TRV ± 0.24 logMAR) than the gold standard ETDRS (TRV ± 0.18 logMAR), but considerably less variable than the Snellen line assignment measurement used in clinical practice (TRV ± 0.33 logMAR). Even when used with a rigorous forced choice testing paradigm, "single letter" measurements using the RLM A chart were completed quite quickly, with a median chart reading time of approximately half that of the equivalent measurements using the ETDRS and Snellen charts. The RLM B and RLM C charts, while quicker still, were more variable. For routine clinical use, the RLM A chart appears to offer a pragmatic compromise trading off TRV against measurement duration. Evidently, the ubiquitous Snellen line assignment method is presently deemed acceptable for clinical use. The RLMA chart offers a lower level of TRV in an average of under 1 minute and the benefits of contemporary logMAR chart designs. It therefore has

great potential for use in routine clinical practice. Having established the potential of this design, further investigations are optimising the chart design in terms of letter spacing, line spacing, and the presence of crowding bars.

- 1 Snellen H. Letterproeven tot Bepaling der Gezigtscherpte (PW van der Weijer 1862) cited in Bennett AG Ophthalmic test types. *Br J Physiol Opt* 1965;22:238-71.
- 2 Bailey I, Lovie J. New design principles for visual acuity letter charts. *Am J Optom Physiol Opt* 1976;53:740-5.
- 3 Sloan LL. Needs for precise measures of visual acuity. *Arch Ophthalmol* 1980;98:286-90.
- 4 Wick B, Schor C. A comparison of crowding bar and linear optotype acuity in amblyopia. *Am J Optom Assoc* 1984;55:359-61.
- 5 Friendly DS, Weiss IP. An automated visual acuity testing computer program using the Apple II system. *Am J Ophthalmol* 1985;99:188-92.
- 6 Elliott D, Sheridan M. The use of accurate visual acuity measurements in clinical anti-cataract formulation trials. *Ophthalm Physiol Opt* 1988;8:397-401.
- 7 Bailey IL, Bullimore MA, Raasch TW, et al. Clinical grading and the effects of scaling. *Invest Ophthalmol Vis Sci* 1991;32:422-32.
- 8 Vanden Bosch ME, Wall M. Visual acuity scored by the letter-by-letter or probit methods has lower retest variability than the line assignment method. *Eye* 1997;11:411-17.
- 9 Sloan LL. New test charts for the measurement of visual acuity at near and far distances. *Am J Ophthalmol* 1959;48:807-13.
- 10 Ferris FL, Kassoff A, Bresnick GH, et al. New visual acuity charts for clinical research. *Am J Ophthalmol* 1982;94:92-6.
- 11 Flom MC, Weymouth FW, Kahneman D. Visual resolution and contour interaction. *Opt Soc Am* 1963;53:1026-32.
- 12 Stager DR, Everett ME, Birch EE. Comparison of linear and optotype acuity in amblyopia. *Am Orthopt J* 1990;40:51-6.
- 13 Bland J, Altman D. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;i:307-10.
- 14 Arditi A, Caganello R. On the statistical reliability of letter-chart visual acuity measurements. *Invest Ophthalmol Vis Sci* 1993;34:120-9.
- 15 Lovie-Kitchen JE. Validity and reliability of visual acuity measurements. *Ophthalm Physiol Opt* 1988;8:363-70.
- 16 Reeves BC, Wood JM, Hill AR. Vistech VCTS 6500 charts—within- and between-session reliability. *Optom Vis Sci* 1991;68:728-37.
- 17 Siderov J, Tiu AL. Variability of measurements of visual acuity in a large eye clinic. *Acta Ophthalmol Scand* 1999;77:673-6.



The development of a "reduced logMAR" visual acuity chart for use in routine clinical practice

D A Rosser, D A H Laidlaw and I E Murdoch

Br J Ophthalmol 2001 85: 432-436

doi: 10.1136/bjo.85.4.432

Updated information and services can be found at:

<http://bjo.bmj.com/content/85/4/432.full.html>

References

These include:

This article cites 13 articles, 3 of which can be accessed free at:

<http://bjo.bmj.com/content/85/4/432.full.html#ref-list-1>

Article cited in:

<http://bjo.bmj.com/content/85/4/432.full.html#related-urls>

Email alerting service

Receive free email alerts when new articles cite this article. Sign up in the box at the top right corner of the online article.

Topic Collections

Articles on similar topics can be found in the following collections

[Public health](#) (377 articles)

Notes

To request permissions go to:

<http://group.bmj.com/group/rights-licensing/permissions>

To order reprints go to:

<http://journals.bmj.com/cgi/reprintform>

To subscribe to BMJ go to:

<http://group.bmj.com/subscribe/>