

'Preferential looking' for monocular and binocular acuity testing of infants

JANETTE ATKINSON, OLIVER BRADDICK, AND ELIZABETH PIMM-SMITH

From the Kenneth Craik Laboratory, University of Cambridge

SUMMARY A method is described for obtaining rapid and reliable estimates of acuity in infants, for both monocular and binocular viewing. The method depends on 'preferential looking', where the infant prefers to look at a striped pattern rather than a blank screen of matched mean luminance. A staircase procedure for testing is followed, with observations being recorded by a 'blind' observer (who does not know on which of the 2 screens the striped pattern is displayed). Monocular acuity estimates have been obtained for a group of infants 3 to 4 months old with normal refractions. Many of these infants show similar acuity values in the 2 eyes, with a few showing reliable differences between the eyes. To check reliability of the method a comparison of 2 independent interleaved staircase estimates of the same eye have been made. In general this check shows highly consistent estimates for a given eye of a given infant. Nearly all infants show slightly higher acuity estimates for binocular viewing than for monocular. The possible reasons for this difference are discussed. The clinical use of such a method is reported for a number of cases. The method has been found to be useful in a variety of clinical conditions where other available tests are not possible on young infants.

The forced-choice preferential looking (FPL) method is now well established as a means of estimating acuity and other visual detection performance in infants aged 1–6 months.^{1–5} The present authors have been using it routinely to assess clinical acuity deficits in this age range, as have others. Published work has generally used FPL with a binocularly viewing infant. However, clinical assessment is usually required for each eye separately. In many instances it is the possible difference between the eyes which is the major concern. Binocular relationships have also been the principal focus of recent work in the developmental neurobiology of vision,^{6,7} and therefore measurements of the performance of each eye separately are required if research on normal and abnormal visual development in infancy is to be related to these studies.

The study reported here was therefore intended to test whether reliable determination of monocular acuity was possible by FPL, what variation of acuity between the eyes would be found in a presumptively normal group of infants using this technique, and

Correspondence to Department of Experimental Psychology, University of Cambridge, Downing Street, Cambridge CB2 3EB.

whether the method would permit the detection of clinically significant interocular differences. As well as these trials of the method on normal infants we describe our experience in the practical use of the method for monocular and binocular testing of infants referred for acuity testing for a variety of clinical reasons.

Material and methods

The apparatus and general procedure resembled that described by Atkinson *et al.*³ Infants were seated on a holder's knee 57 cm from a pair of oscilloscope screens, at which distance the diameter of each screen subtended 10.5° and the separation of the screens 6.3°. Between trials both screens displayed a uniform field of luminance 30 cd/m², and a set of lights midway between the screens attracted the infant's attention. A concealed observer watched the infant from a central peephole above the screens, and initiated a trial when the infant was fixating centrally. During the trial one of the screens (selected automatically at random) was modulated by a high-contrast horizontal sinusoidal grating while the other remained uniform and of equal mean luminance. (The gratings moved

steadily with a temporal modulation rate of 3 Hz.) The observer was unaware of which side the grating was displayed and had to make a forced choice of this based on observation of the infant's fixations and other behaviour. The duration of the observation period necessary for this was under the observer's control up to maximum of 10 seconds and was typically 5 seconds or less for infants of the age tested in this study. If on any trial an infant was not looking at either screen the observer could abandon that trial without having to make a forced-choice judgment.

For monocular testing an adhesive orthoptic patch was placed over the left or right eye. The observer checked the alertness and lack of fussiness of the infant by presenting a low spatial frequency grating (0.5 c/deg), and checking that the infant made a clear observable eye movement to the display on the side of the pattern. The infant's position in front of the screens was arranged so that before the pattern was presented the viewing eye was in line with the central fixation lights.

A series of spatial frequencies (grating stripe widths) were chosen in which each frequency was higher than the one below by a factor of 1.6 (two-thirds octave). Testing was started with 5 trials using a grating of 2 c/deg. After this the spatial frequency used for each block of 5 trials was selected according to a 'staircase' rule.⁸ That is, if on the previous block the observer had made 4 or 5 correct choices the spatial frequency was increased by one step for the next block. Two or fewer correct choices led to the next lowest spatial frequency being used in the next block. If there were 3 correct choices out of 5, the

frequency remained unchanged; if this occurred on 3 successive blocks, the next frequency was chosen in the direction most likely to meet the criterion for completing the staircase.

A staircase was taken as complete when at least 20 trials had been run at each of 2 adjacent frequencies, with the proportion of correct responses bracketing or including the value of 70%. Normally between 50 and 90 trials were needed to meet this criterion. The acuity value was taken as the 70% point obtained by interpolation between these 2 spatial frequencies.

To test acuity of the 2 eyes under conditions which were as comparable as possible in terms of the infant's state we used a method of 'interleaved staircases.' Twenty-five trials (i.e., 5 blocks) were run with one eye occluded; the occluding patch was then switched to the other eye and a new staircase sequence was followed for 25 trials.

The patch was then put back on the first eye, the next block of 25 trials followed the original staircase from where it had been left off, and so on. An example of the procedure is illustrated in Fig. 1. To assess the reproducibility of measurements made with our technique we tested some other infants with the same procedure of 2 interleaved staircases but with both independent staircase sequences testing the same eye. We shall refer to this as 'series 1/series 2 comparison.'

The infants volunteered by their parents to help in this study were from the Cambridge area. All infants had normal birth histories and were not more than 10 days premature. The mean age of testing on the first visit was 16 weeks (3½ months). Testing on each

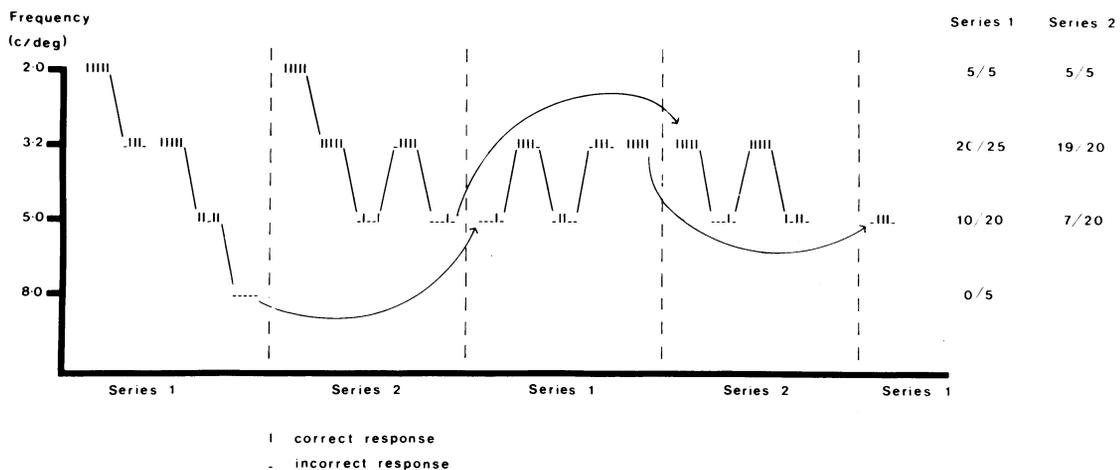


Fig. 1 An example of the procedure used for infants who were tested with 2 independent staircases on one eye to obtain 2 interleaved estimates of acuity.

child was completed within a period of 14 days. To complete the testing most infants made 3 visits; a few completed testing in 2 visits and a few took up to 5 visits. They were tested when alert and calm, usually after a feed. No testing period was longer than 15 minutes.

All the infants were photorefracted under conditions of free accommodation⁹ to detect any refractive errors which might affect the comparisons being made. No infant showed any difference between the eyes greater than 0.5 D in any meridian.

Twenty-nine infants were tested in all, of whom 4 did not complete monocular testing because of fussiness and so are not included in the results. The remaining 25 received different conditions of testing in various sequences, outlined in the results section.

Results

Sixteen infants received interleaved staircases viewing with the left and right eyes. The acuity values obtained are indicated by solid circles on Fig. 2. This figure also includes data from 7 infants for whom each eye was tested but not in interleaved staircases, because they were initially in the group for series 1/series 2 comparison (open circles on Fig. 2). In most cases measurements on the 2 eyes showed good agreement (i.e., the points lay close to the 45° line). The median ratio of measured acuity between the eyes (ratios always taken as greater than 1.0) was 1.12. However, a few individuals showed a more marked interocular difference, which was as large as 2.0 in 2 cases.

To estimate the reliability of these figures we have the comparisons of series 1/series 2 shown in Fig. 3. These data are from 6 infants for whom series 1/series 2 were interleaved for one eye, and from each eye of 3 further infants for whom series 1/series 2 were obtained on both eyes. (Data from the latter infants are included in Fig. 2 also.) All data points lay very close to the 45° line (median acuity ratio for the two series=1.06; maximum ratio=1.20). It appears therefore that the variations seen in Fig. 2 are not a consequence of variability in the method but reflect the range of genuine interocular differences at this age.

Fig. 4 shows the results of comparing binocular and monocular acuity determinations on the same infants. The monocular acuity shown was the better of the 2 values for each infant except in the 2 cases represented by open circles, in which only one eye received monocular testing. None of the binocular testing was interleaved with monocular testing. In general the estimated binocular acuities were higher than the better monocular acuities. There are several possible reasons for this difference between

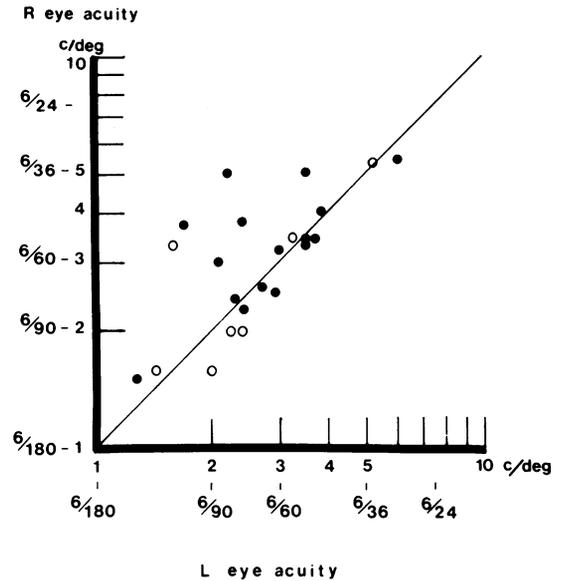


Fig. 2 Acuity estimated for R and L eyes of 23 infants. The filled circles are infants where the 2 eyes' estimates were interleaved, the open circles are for noninterleaved results. Outer scales give Snellen equivalent of the acuity measures.

Monocular Acuity - repeated series on same eye

acuity - Series 2

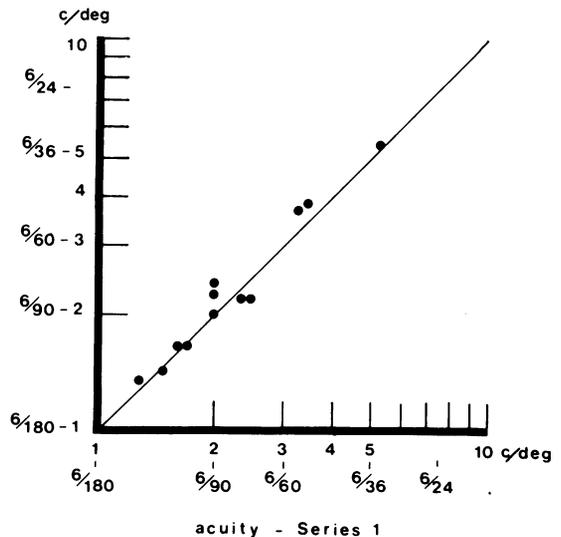


Fig. 3 Comparison of 2 acuity estimates with the same eye for 12 eyes from individual infants. The 2 estimates were interleaved in blocks of 25 trials.

Discussion

The results of Figs. 2 and 3 show that reliable monocular estimates of acuity are possible with infants by the preferential looking (PL) method, although it demands more attention to infant handling than binocular use of the same method. PL is therefore suitable for clinical assessment of monocular as well as binocular disorders of infant vision. But we have also shown measurable differences in interocular acuity in presumptively normal 3-month-olds. The reason for these differences is not known. However, it is perhaps not surprising that in a period of rapid acuity development¹⁰ the 2 eyes might sometimes be found to be at slightly different stages of that development. We presume that such differences are transient. Acuity differences of a factor of more than 2, or differences that persist, may be considered as probable indications of abnormality.

In the PL procedure to assess acuity in clinical cases we find it more successful in infants under 9 months (or equivalent developmental age) than in older infants. Estimates are often possible for the older infants, but it is frequently not possible to maintain the infant's attention long enough to complete the staircase procedure described here. We hope that it may prove possible to apply more sophisticated statistical procedures to PL testing^{11 12} and thereby reduce the number of trials necessary to achieve a reliable threshold estimate.

There is still a great need for a robust test suitable for children over 9 months but too young for subjective tests such as the Sheridan-Gardiner. The tracking tests such as Catford drum¹³ and Stycar balls¹⁴ suffer from some shortcomings in target design and procedure.¹⁵ We are currently exploring the application of tests which depend on tracking but use stimuli that are genuine resolution targets, and which maintain the principles of forced choice by a blind observer and staircase determination of threshold which we have applied in the PL test.

This work was supported by the Medical Research Council. We would like to thank our clinical colleagues from the Department of Ophthalmology (especially Mr P. G. Watson and Mr J. Keast-Butler) and the Department of Paediatrics, Addenbrooke's Hospital, Cambridge, for referring their infants to us and for helpful discussions of the results.

References

- 1 Teller DY, Morse R, Borton R, Regal D. Visual acuity for vertical and diagonal gratings in human infants. *Vision Res* 1974; **14**: 1433-9.
- 2 Teller DY. The forced-choice preferential looking procedure: a psychophysical technique for use with human infants. *Infant Behav Devel* 1979; **2**: 135-53.
- 3 Atkinson J, Braddick O, Moar K. Development of contrast sensitivity over the first 3 months of life in the human infant. *Vision Res* 1977; **17**: 1037-44.
- 4 Banks MS, Salapatek P. Acuity and contrast sensitivity in 1-, 2-, and 3-month-old human infants. *Invest Ophthalmol Visual Sci* 1978; **17**: 361-5.
- 5 Gwiazda J, Brill S, Mohindra I, Held R. Infant visual acuity and its meridional variation. *Vision Res* 1978; **18**: 1557-64.
- 6 Hubel DH, Wiesel TN. Functional architecture of macaque monkey visual cortex. *Proc R Soc Lond (Biol)* 1977; **198**: 1-59.
- 7 Blakemore C. Maturation and modification in the developing visual pathway. In: Held R, Leibowitz HW, Teuber HL, eds. *Handbook of Sensory Physiology: Perception*. Berlin: Springer, 1978; **8**.
- 8 Cornsweet TN. The staircase method in psychophysics. *Am J Psychol* 1962; **75**: 485-91.
- 9 Braddick OJ, Atkinson J, French J, Howland HC. A photo-refractive study of infant accommodation. *Vision Res* 1979; **19**: 1319-30.
- 10 Dobson V, Teller DY. Visual acuity in human infants: a review and comparison of behavioural and electrophysiological studies. *Vision Res* 1978; **18**: 1469-83.
- 11 Taylor MM, Creelam CD. PEST: Efficient estimates on probability functions. *J Acoust Soc Am* 1967; **41**: 782-7.
- 12 Watson AB, Pelli DG. The Quest staircase procedure. *AVA Newsletter* 1979; no. 14.
- 13 Catford GV, Oliver A. Development of visual acuity. *Arch Dis Child* 1973; **48**: 47-50.
- 14 Sheridan MD. *Manual for the STYCAR vision tests*. NFER Publishing Company, 1976.
- 15 Braddick OJ, Atkinson J, Pimm-Smith E, Ayling L, Sawyer R. Does the Catford drum give an accurate assessment of acuity? *Br J Ophthalmol* 1981; **65**: 652-6.